



Sea-Bird Electronics, Inc.  
 1808 136th Place NE  
 Bellevue, WA 98005  
 USA

Phone: (425) 643-9866  
 Fax: (425) 643-9954  
 E-mail: seabird@seabird.com  
 Web: www.seabird.com

**APPLICATION NOTE NO. 70**

**Revised October 2006**

**Installing Anti-Foulant Device Mount Kit  
 on SBE 4, 16, 19, and 21 Conductivity Cells**

This application note applies to the SBE 4 conductivity cell (used in a moored application), SBE 16 (not 16*plus*) SEACAT, SBE 19 (not 19*plus*) used in moored mode, and SBE 21 SEACAT Thermosalinograph.

**Note:** The SBE 4 is integrated with the SBE 26 SEAGAUGE Wave and Tide Recorder, SBE 26*plus* SEAGAUGE Wave and Tide Recorder, or SBE 53 BPR Bottom Pressure Recorder if the Recorder includes an optional conductivity sensor.

**Part number 50315 is an external anti-foulant device mount kit.** The kit contains:

Part Number	Description
231505	anti-foulant device caps (2)
231513	external in-line anti-foulant device cups (2)
30579	3/8 inch ID, 1/2 inch OD Tygon tube (6 cm long)



Anti-foulant device cup      Anti-foulant device cap


Order the PN 50315 mount kit and PN 801542 AF24173 Anti-Foulant Devices the first time you need Anti-Foulant Devices. Once you have the kit, you only need to order the AF24173 Anti-Foulant Devices.

**External Anti-Foulant Device Mount Kit Installation Procedure**

1. Cut two 3-cm long pieces from the Tygon tubing.
2. Place the barbed end of the anti-foulant device cup inside the Tygon tubing.
3. Screw the anti-foulant device cap in place. Do not over tighten.
4. Carefully slide the Tygon tubing over the end of the conductivity cell. **Do not apply any sideways or twisting motion to the end of the conductivity cell, or you may damage the cell.**
5. Repeat Steps 2 through 4 for the other end of the conductivity cell.



Tygon tubing and anti-foulant device cup and cap

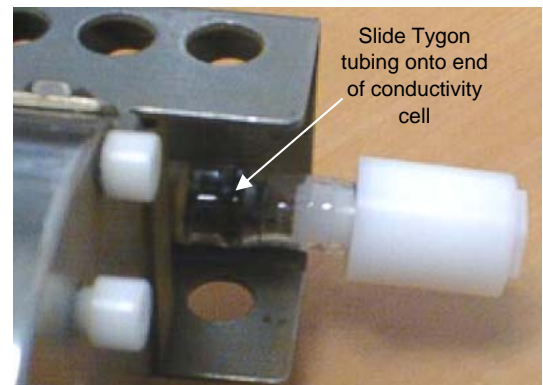

SBE 21 shown; SBE 4, 16, and 19 similar